

## Determination of Bisphosphonates by Ion-pair HPLC

Matuszewski, Łukasz

Department of Pediatric Orthopedy and Rehabilitation, Medical University of Lublin

Matuszewska, Anna

Department of Biochemistry, Maria Curie-Skłodowska University

Mazurkiewicz, Tomasz

Department of Orthopedy and Traumatology, Medical University of Lublin

Rogalski, Jerzy

他

<https://doi.org/10.5109/20311>

---

出版情報：九州大学大学院農学研究院紀要. 56 (2), pp.213-216, 2011-09. Faculty of Agriculture, Kyushu University

バージョン：

権利関係：



## Determination of Bisphosphonates by Ion-pair HPLC

**Łukasz MATUSZEWSKI<sup>1</sup>, Anna MATUSZEWSKA<sup>3</sup>, Tomasz MAZURKIEWICZ<sup>2</sup>,  
Jerzy ROGALSKI<sup>3</sup>, Nam-Seok CHO<sup>4</sup> and Shoji OHGA\***

Laboratory of Forest Resources Management, Division of Forest Environmental Sciences,  
Department of Agro-environmental Sciences, Faculty of Agriculture,  
Kyushu University, Sasaguri, Fukuoka 811-2415, Japan  
(Received April 4, 2011 and accepted May 9, 2011)

The optimization of the two bisphosphonates (disodium pamidronate and zoledronic acid) separation by ion-suppression and ion-pair high-performance liquid chromatography is described. The influence of the eluent pH, composition of the mobile phase and the concentration of complexing ion-pairing agents was investigated. This developed method provides high separation and specificity to bisphosphonate analysis. In quantitative analysis in the optimized conditions (10 mM n-amylamine or n-butylamine; 14% acetonitrile in 0.1 M sodium phosphate buffer, pH=7.0), the method showed good linearity ( $r=0.9999-0.9998$ ) and sufficient sensitivity ( $10^{-7}-10^{-8}$  g/ml). It can be easily and conveniently adopted for the routine quality control analysis.

### INTRODUCTION

Bisphosphonates are a broad class of synthetic compounds possessing a P–C–P bridge structure and are typically used to inhibit bone resorption. They are extensively used in the management of skeletal disorder including osteoporosis, malignant hypercalcemia, bone metastasis and Paget's disease (Sparidans and Hartigh, 1999). Bisphosphonates play an important role in aseptic environment of total joint replacements and may contribute to the *in vivo* longevity of total joint replacements. Some data suggest that they can decrease in flexural strength and flexural modulus of cured cement (Lewis and Janna, 2006). When these compounds have been administered to the patient they have two possibilities of their delivery options *e.g.* systematic (oral ingestion or intravenous injection) (Morris and Einhorn, 2005) or local (Sabokbar *et al.*, 1998). It has been shown that oral administration of bisphosphonates can be used to reduce osteoclastic reaction to wear debris and the resultant resorption in arthroplasty surgery (Antoniou *et al.*, 2000). Local delivery system is that bisphosphonates are mixed with bone cement coating deposited implants (Peter *et al.*, 2005). This delivery method must be carefully tested in some ways. First the clinical studies must determine the kind of specific bisphosphonate, mode of its delivery and dosage. Next the mechanism(s) of its action on cultures of osteoblast cells on human bone slices as well as the influence of this compound on the properties of the cured cement must be determined.

The details of bisphosphonate leaking from the cured cement into a biosimulating solution must be also evaluated (Lewis and Janna, 2005). The bisphosphonate drugs are also used in veterinary for the suppression of bone remodeling and tumor osteolysis as a palliative treatment of animals with osteosarcoma (Tomlin *et al.*, 2000; Ashlon *et al.*, 2005).

The chemical nature of bisphosphonates causes some analytical difficulties. These compounds are strongly polar and ionic that causes a problem with their extraction from biological fluids into an organic solvent and they are no volatile (Sparidans and Hartigh, 1999).

The method that has been used so far for the investigation of these compounds are non-chromatographic methods based on either titration with thorium diamino-cyclohexanetetra acetate (Liggett, 1973) or on detection of phosphate as a triethylamine-phosphomolybdate complex after decomposition of the bisphosphonate (Bisaz *et al.*, 1975). The newest class of bisphosphonates which are used in lower doses increase the demands on the sensitivity of the analysis which can be only realized by chromatographic methods (Fleisch, 1991). For the development of analytical separation methods, several strategies have been followed mainly IEC (ion-exchange chromatography) (Daley-Yates *et al.*, 1989), and reversed-phase liquid chromatography (RPLC) (Kwong *et al.*, 1990) often in combination with an ion-pairing agent. Gas chromatography technique is rather limited due to difficulties in transferring the ionic bisphosphonate into an organic solvent (Auriola *et al.*, 1989). Recently capillary electrophoretic (CE) separations have also been described (Huikko and Kostinen, 2000).

In this investigation, the conditions for the separation of two bisphosphonates were examined and optimized. N-amylamine, n-butylamine or tetrabutyl-ammonium chloride was used as the complexing agent (counter ion). The influence of the eluent pH, counter-ions concentration, and the amount of methanol and acetonitrile in the mobile phase was also examined (Bidlemeier, 1980; Xie *et al.*, 2006).

<sup>1</sup> Department of Pediatric Orthopedy and Rehabilitation, Medical University of Lublin, Chod ki 2 Str., 20-093 Lublin, Poland

<sup>2</sup> Department of Orthopedy and Traumatology, Medical University of Lublin, Jaczewskiego 8 Str., 20-954 Lublin, Poland

<sup>3</sup> Department of Biochemistry, Maria Curie-Skłodowska University, Langiewicza 19 Str., 20-031 Lublin, Poland

<sup>4</sup> Wood and Paper Science, Chungbuk National University, Cheongju 361-763, Korea

\* Corresponding author: (E-mail: ohga@forest.kyushu-u.ac.jp)

## MATERIALS AND METHODS

## Chemicals

*Pamidronate* (3-amino-1-hydroxypropylidene) bis-phosphonate SIGMA (St.Louis, USA) (HPLC standard) and clinical preparation from Vipha S.A. (Warszawa, Poland), zoledronic acid [1-hydroxy-2-(1H-imidazole-1-yl) ethylidene] bis-phosphonate was obtained from LKT Lab. (St.Paul, USA) (HPLC standard) and Novartis (Nürnberg, Germany). Acetonitrile and methanol HPLC grade were purchased from Merck (Darmstadt, Germany). N-butylamine, n-amylamine were obtained from Sigma (St.Louis, USA) and tetrabutyl-ammonium chloride was obtained from Fluka (Buchs, Switzerland). For mobile phase preparation MilliQ water was used.

Stock standard solutions of pamidronate and zoledronic acid (1 mM) were prepared by dissolving in water. Each solution was further diluted to obtain a series of working standards, pipetted into 500  $\mu$ l Eppendorf tubes and frozen under liquid nitrogen. Because of instability of investigated substances all standard solutions after defrosting were used only 12 hours.

## Equipment and chromatographic conditions

HPLC analysis was carried out using the reversed-phase column Phenomenex Luna C<sub>18</sub>(2) column (250 mm  $\times$  4.6 mm I.D.), particle size 5  $\mu$ m and was protected by a Phenomenex Security Guard column. The chromatographic system consisted LC-9A precision pump (Shimadzu, Japan), an SPD-M10A diode array detector and a Model 7125 sampling valve RHEODYNE (Berkeley, USA) with 20  $\mu$ l loop and was controlled by Shimadzu Class M10A Work Station (v.1.64). The mobile phase used was a mixture of (2–36 mM n-amylamine or n-butylamine or tetrabutylamine chloride aqueous solution (adjusted to pH 5–8.5 with acetic acid) and acetonitrile (2–30%) or methanol (2–44%) (v/v). The flow-rate was 0.5 ml/min and all experiments were done at room temperature. The spectra of tested substances were determined in a Shimadzu UV-VIS 160A spectrophotometer (Shimadzu, Tokyo, Japan) controlled by Pentium IV PC computer with PC 160 plus software.

## RESULTS AND DISCUSSION

The choice of the chromatograph detector in high performance liquid chromatography as well as physical properties measured substances in the column eluate influence for the detection limits. Bisphosphonates in LC can be detected by direct sensitive detection like UV adsorption, fluorescent and/or ability to oxidation (Peng *et al.*, 1998; Sparidans and Hartigh, 1999). Sometimes a chromatographic separation has been preceded by one or more pretreatment steps as derivatization which enhance the detectability and/or to improve the selectivity of the separation (Fruitier *et al.*, 1990; Lovdahl and Pietrzyk, 1999; Perez-Ruiz *et al.*, 2009).

In the first step of the experiments we have checked the spectra of disodium pamidronate and zoledronic acid looking for the possibility of using UV-VIS detector.

In the both cases the high absorption were observed in near UV region about 210 nm which was chosen as the length of wave for chromatographic detector in the next experiments. The stability of clinical used preparates was checked after 1, 3, 6, 12, 24, 48 and 72 hours by measuring their spectra profiles from 200 to 400 nm. The obtained profiles of disodium pamidronate and zoledronic acid specialty clinical grade after 24 hours showed a small unstabilities and for this reason we have used fresh solution only for 12 hours.

All the bisphosphonates are strongly polar and ionic that do not give sufficient retention on the hydrophobic stationary phase such as C<sub>18</sub> or C<sub>8</sub> (Niemi *et al.*, 1997; Xie *et al.*, 2006). Very helpful for this reason is application of an ion-pairing agent which can increase the bisphosphonates retention on this kind of the sorbent. In our investigation we have used tetrabutylammonium chloride (Sparidans and Hartigh, 1999) or n-amylamine (Xie *et al.*, 2006) or n-butylamine (Niemi *et al.*, 1997) as ion-pair reagent. These compounds (oppositely charged ions) may combine with bisphosphonates to the form of neutral ion-pair, which can be retained on nonpolar stationary phase.

Optimization of separation conditions of the test mixture of two bisphosphonates was carried out in three stages: (a) choice of the complexing agent concentration; (b) determination of the optimal composition of the mixed mobile phase (organic compound–buffer) and (c) effect of mobile phase pH.

The effect of ion-pair agents (tetrabutylammonium chloride (TBA), n-amylamine and n-butylamine) concentration on the retention (*k*–retention factor) of disodium pamidronate and zoledronic acid at constant pH (7.0) and organic modifier (acetonitrile 5%) is shown in Table 1. The retention of tested bisphosphonates increased with increasing from 2 to 36mM ion-pairing agents con-

**Table 1.** Influence of complexing agents concentration on *k* of disodium pamidronate and zoledronic acid

Complexing agent and its concentration [mM]	k value	
	Disodium pamidronate	Zoledronic acid
n-amylamine	2	1.40
	10	1.67
	18	1.92
	26	2.10
	36	2.28
n-butylamine	2	1.92
	10	1.96
	18	2.00
	26	2.08
	36	2.15
tetrabutylammonium chloride	2	2.94
	10	3.01
	18	3.09
	26	3.54
	36	4.07

centrations. Satisfied separations of tested compounds were obtained when concentration of *n*-amylamine as well *n*-butylamine was 10 mM. The higher concentration of these complexing agents as well using TBA caused baseline drift and increase in background noise. For this reason, in the next experiments *n*-amylamine at 10 mM concentration as ion-pair reagen was chosen.

The next step of this work was determination of an organic modifier (acetonitrile 2–30% and methanol 2–44%) composition in mobile phase on the retention of disodium pamidronate and zolendronic acid at constant concentration of *n*-amylamine (10 mM) and constant pH (7.0) of mobile phase (Fig. 1).


Replacement of methanol with acetonitrile led to lower *k* values and even to shorter analysis time. In the case when methanol was used the chromatographic peaks were shown much more deformation. Sometimes asymmetry factors value were higher than 1.2 (data not shown) what exceed the acceptable value (Suprynowicz *et al.*, 1984). For these reason the acetonitrile in the concentration 14% was chosen for further studies.

Bisphosphonates belonging to quadribasic acids having several  $pK_a$  values that capable of forming multiply charged ions in solution. Therefore, the pH level of mobile phase is very important parameter in the ion-pair


HPLC for analysis of bisphosphonates because of the significant effect on the retention behaviour and peak shape. The retention factor of test mixture compounds were measured for different eluent pH (5–8.5) at the constant concentration of ion-pairing modifying agents (10 mM) and 14% acetonitrile Fig. 2. The retention of tested bisphosphonates clearly increased parallelly to the increasing eluent pH. At pH 7.0 the differences in *k* value of disodium pamidronate and zolendronic acid was so big as in higher values and we have obtained not only good separation but also short time of analysis. The similar results in the optimization procedure of four different bisphosphonates were obtained by (Xie *et al.*, 2006).

The detection limits of pamidronate and zolendronic acid obtained in the optimized condition are compared in Table 2. As we can see in the case of zolendronic acid and disodium pamidronate detection limit was about  $10^{-7}$ – $10^{-8}$  g/ml *e.g.* 10 to 100 times lower to compare with Xie *et al.* (2006) method where the ELSD detector was used.

Results from assay of disodium pamidronate and zolendronic acid in bulk material are shown in Table 3. The precision of the data and the agreement between the label claim and the found amount were very high. Ingredients of commercially available samples did not

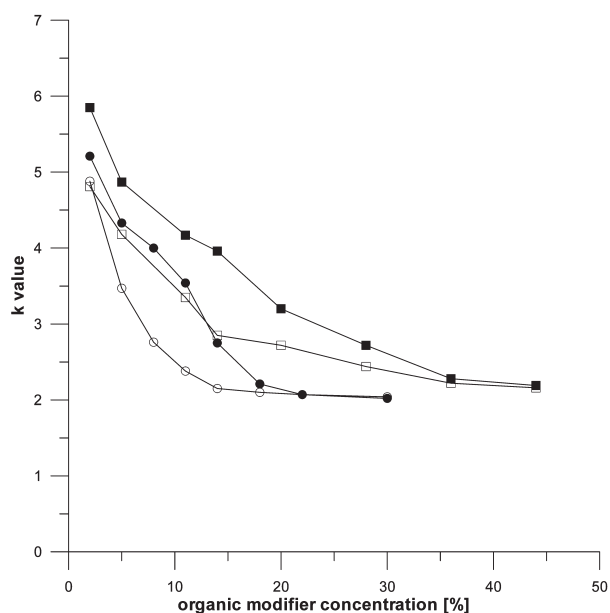

**Fig. 1.** The dependence of pamidronate (○, ●) and zolendronic acid (□, ■) retention factors (*k*) on the amount of acetonitrile (○, □) or methanol (●, ■) in mobile phase.

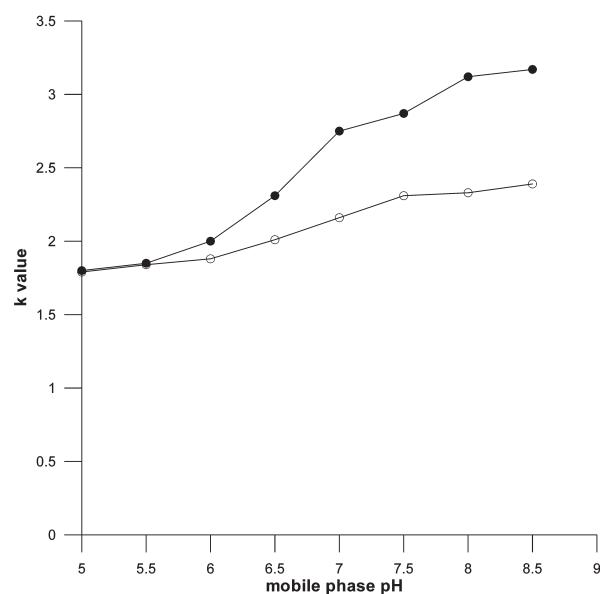

**Fig. 2.** Influence of mobile phase pH on retention factors (*k*) of pamidronate (○) and zolendronic acid (□).

**Table 2.** Linear regression calibration and detection limit data for bisphosphonates

Compound	Concentration range [ $\mu\text{g/ml}$ ]	Regression line	Corelation coefficient [ <i>r</i> ]	Detection limit [ $\mu\text{g/ml}$ ]
Disodium pamidronate	0.05–1000	$y = 1.2299x - 6.266$	0.9999	0.115
Zolendronic acid	0.05–1000	$y = 1.1346x + 2.087$	0.9998	0.064

**Table 3.** Analysis of bisphosphonates samples

Product	N	Claim amount [%]	Found amount in standart [%]
Disodium pamidronate	5	100.00	98.78±1.91
Zolendronic acid	5	100.00	97.57±2.27

interfere with analytes. Under the chromatographic analytical procedure we can easily determined these components with so high resolution in standard solution as well as in clinical samples.

### REFERENCES

- Antoniou, J., O. Huk, D. Zukor, D. Eyre and M. Alini 2000 Collagen crosslinked N-telopeptides as markers for evaluating particulate osteolysis: a preliminary study, *J. Orthop. Res.*, **18**: 64–67
- Ashton, J. A., J. P. Farese, R. J. Milner, L. M. Lee–Ambrose and J. M. vanGilder 2005 Investigation of the effect of pamidronate disodium on the in vitro viability of osteosarcoma cells from dogs, *Am J. Vet. Res.*, **66**: 885–891
- Auriola, S., R. Kostianen, M. Yienen, J. Mönkkönen and P. Yitalo 1989 Analysis of (dichloromethylene) bisphosphonate in urine by capillary gas chromatography–mass spectrometry, *J. Pharm. Biomed. Anal.*, **7**: 1623–1629
- Bidlingmeyer, B. A. 1980 Separation of ionic compounds by reversed–phase liquid chromatography: an update of ion–pairing techniques, *J. Chromatogr. Sci.*, **18**: 525–539
- Bisaz, S., R. Felix and H. Fleisch 1975 Quantitative determination of ethane–1–hydroxy–1, 1–diphosphonate in urine and plasma, *Clin. Chim. Acta*, **65**: 299–307
- Fleisch, H. 1991 Bisphosphonates. Pharmacology and use in the treatment of tumor–induced hypercalcaemic and metastatic bone disease, *Drugs*, **42**: 919–944
- Fruitier, A. N., W. J. M. Underberg, H. Lingeman and J. H. Beijnen 1990 Derivatization reactions and kinetics in liquid chromatography. In: Detection–oriented derivatization techniques in liquid chromatography (H. Lingeman and W. J. M. Underberg, eds.), New York, Mercel Dekker Inc., pp. 51–84
- Gilford, L. A. and C. R. Hoggarth 1989 Assay of 1–hydroxy–3–aminopropylidene–1,1–bisphosphonate and related bisphosphonates in human urine and plasma by high–performance ion chromatography, *J. Chromatogr.*, **490**: 329–338
- Huikko, K. and R. Kostianen 2000 Analysis of bisphosphonates by capillary electrophoresis–electrospray ionization mass spectrometry, *J. Chromatogr.*, **872**: 289–298
- Kwong, E., A. M. Y. Chiu, S. A. McClintock and M. L. Cotton 1990 HPLC analysis of an amino bisphosphonate in pharmaceutical formulations using post–column derivatization and fluorescence detection, *J. Chromatogr. Sci.*, **28**: 563–566
- Lewis, G. and S. Janna 2006 Aldendronate in bone cement, *Clin. Orthop. Rel. Res.*, **445**: 233–238
- Liggett, S. J. 1973 Determination of ethane–1–hydroxy–1,1–diphosphonic acid (EHDP) in human feces and urine, *Biochem. Med.*, **7**: 68–77
- Lovdahl, M. J. and D. J. Pietrzyk 1999 Anion–exchange separation and determination of bisphosphonates and related analytes by post–column indirect fluorescence detection, *J. Chromatogr.*, **850**: 143–152
- Morris, C. D. and T. A. Einhorn 2005 Bisphosphonates in orthopedic surgery, *J. Bone Joint Surg.*, **87**: 1609–1618
- Niemi, R., H. Taipale, M. Ahlmark, J. Vepsäläinen and T. Järvinen 1997 Simultaneous determination of clodronate and its partial ester derivatives by ion–pair reversed–phase high–performance liquid chromatography coupled with evaporative light–scattering detection, *J. Chromatogr. B.*, **701**: 97–102
- Peng, S. X., R. Takigiku, D. E. Burton and L. L. Powell 1998 Direct pharmaceutical analysis of bisphosphonates by capillary electrophoresis, *J. Chromatogr.*, **709**: 157–160
- Perez–Ruiz, T., C. Martinem–Lozano and M. D. Garcia–Martinez 2009 A sensitive post–column photochemical derivatization/fluorimetric detection system for HPLC determination of bisphosphonates, *J. Chromatogr.*, **1216**: 1312–1318
- Peter, B., D. P. Pioletti, S. Laib, B. Bujoli, P. Pilet, P. Janvier, J. Guicheux, P. Y. Zambelli, J. M. Boulter and O. Gauthier 2005 Calcium Phosphate drug delivery system: influence of local zolendronate release on bone implant osteointegration, *Bone*, **36**: 52–60
- Sabokhar, A., Y. Fyjikawa, D. Murray, N. Athanasou 1998 Bisphosphonates in bone cement inhibit PMMA particle induced bone resorption, *Ann. Rheum. Dis.*, **57**: 614–618
- Sparidans, R. W. and J. Hartigh 1999 Chromatographic analysis of bisphosphonates, *Pharm. World Sci.*, **21**: 1–10
- Supryniewicz, Z., B. Buszewski, J. Rogalski and E. Malarczyk 1984 Determination of veratric acid and its metabolites in biological material by ion–pair high–performance liquid chromatography, *J. Chromatogr.*, **286**: 253–260
- Tomlin, J. L., C. Sturgeon, M. J. Pead and P. Muir 2000 Use of bisphosphonate drug aldendronate for palliative management of osteosarcoma in two dogs, *Vet. Rec.*, **147**: 129–132
- Xie, Z. X., Y. Jiang and D. Q. Zhang 2006 Simple analysis of four bisphosphonates simultaneously by reverse phase liquid chromatography using n–amylamine as volatile ion–pairing agent, *J. Chromatogr.*, **1104**: 173–178