

New solutions for automated image recognition and identification: Challenges to radiologic technology and forensic patholog

Morishita, Junji

Department of Health Sciences, Faculty of Medical Sciences, Kyushu University

Ueda, Yasuyuki

Department of Medical Physics and Engineering, Area of Medical Imaging Technology and Science, Division of Health Sciences, Graduate School of Medicine, Osaka University

<https://hdl.handle.net/2324/4400028>

出版情報 : Radiological Physics and Technology, 2021-03-12. Springer

バージョン :

権利関係 :

Review

1 **New solutions for automated image recognition and identification: Challenges to**
2 **radiologic technology and forensic pathology**

3

4 Junji Morishita¹ and Yasuyuki Ueda² (co-corresponding authors)

5

6 1 Department of Health Sciences, Faculty of Medical Sciences, Kyushu University

7 3-1-1 Maidashi, Higashi-ku, Fukuoka, Fukuoka 812-8582 Japan

8 morishita.junji.894@m.kyushu-u.ac.jp

9 092-642-6673

10

11 2 Department of Medical Physics and Engineering, Area of Medical Imaging

12 Technology and Science, Division of Health Sciences, Graduate School of Medicine,

13 Osaka University

14 1-7 Yamadaoka, Suita, Osaka 565-0871, Japan

15 ueda@sahs.med.osaka-u.ac.jp

16 06-6879-2443

17 **Abstract**

18 This paper outlines the history of biometrics for personal identification, the current status
19 of the initial biological fingerprint techniques for digital chest radiography, and patient
20 verification during medical imaging, such as computed tomography and magnetic
21 resonance imaging. Automated image recognition and identification developed for
22 clinical images without metadata could also be applied to the identification of victims in
23 mass disasters or other unidentified individuals. The development of methods that are
24 adaptive to a wide range of recent imaging modalities in the fields of radiologic
25 technology, patient safety, forensic pathology, and forensic odontology is still in its early
26 stages. However, its importance in practice will continue to increase in the future.

27 (110 words)

28

29

30 **Key words:** image recognition, biometrics, biological fingerprints, biometric verification,
31 positive identification, forensic identification

32 **1. History of personal identification using biometrics**

33 Personal identification using fingerprinting, DNA analysis, and dental records has been
34 used for multiple purposes, such as forensic identification and identity verification.
35 Several researchers, including medical examiners/coroners, forensic pathologists, and
36 forensic anthropologists, are continually working to establish standards and systematic
37 analysis methods for application to unknown cases and human remains [1]. However,
38 daily activities often require rapid, reliable, and convenient personal identification. Thus,
39 personal identification is becoming the fundamental of today's society, and ongoing
40 research contributes more secure services to prevent fraud and crime while improving
41 accessibility and convenience.

42 Research regarding personal identification using biometrics originated in the 1600s,
43 when human fingerprint patterns were used. In 1684, Grew conducted extensive research
44 on the ridge patterns of fingerprints to distinguish different human beings [2]. In 1685,
45 Bidloo described the details of the fingerprint in the book *Anatomy of the Human Body*
46 [3]. Around that time, the fact that fingerprint patterns are unique to individuals began to
47 be recognized. Mayer wrote a book in 1788, entitled *Anatomical Copper-plates with*
48 *Appropriate Explanations*, asserting that the pattern of fingerprints is unique to each
49 human [4]. He wrote, "Although the arrangement of skin ridges is never duplicated in two

Review

50 persons, nevertheless the similarities are closer among some individuals.” The differences
51 have been well identified; despite all persons having similar patterns, the specific
52 arrangements show slight differences [5]. Thus, fingerprints were applied as the first
53 commercially available biometric identification method in 1858 by Herschel, who
54 prompted local Indian businessmen to sign binding contracts with a print of their own
55 palm. The fingerprint was used as a system of identification equivalent to official
56 signatures in the magistrate court [6]. In the late 1800s, although not yet fingerprint
57 authorization, Bertillon reported that the combination of 11 anthropometric
58 measurements was unique to the individual [7]. That was the first attempt to use specific
59 anatomical characteristics to identify reoffending criminals. As for the criminal history
60 records in the Justice system, Galton developed a fingerprint-classification system and
61 published a book, *Finger Prints*, in 1892 [8]. Edward Richard Henry published
62 *Classification and Uses of Finger Prints* in 1900 [9]. In 1903, fingerprinting was used to
63 identify prisoners in the New York State Prison. Subsequently, an increasing number of
64 local police identification bureaus established fingerprint systems [10, 11]. In 1986, the
65 National Bureau of Standards (NBS) and the American National Standards Institute
66 (ANSI) published a standard for the exchange of fingerprint minutiae (ANSI/NBS-ICST
67 1-1986). However, personal identification using biometrics was implemented manually,

68 at that time, without the numerical computation of biometric characteristics.

69 Image recognition for personal identification is rapidly progressing with image
70 digitization and evolution in computer vision. There is no doubt that computers can
71 identify images in a shorter time for a greater number of samples with higher accuracy
72 than humans can. **Figure 1** shows several practical features that are commonly
73 implemented for biometric information. It is important to note that several features,
74 including those for biometric technology, are still in varying stages of development and
75 assessment.

76

77 **2. Environment and patient safety in medical imaging**

78 In 1982, Dwyer *et al.* proposed the concept of a picture archiving and communication
79 system (PACS) to reduce the cost of medical image management [12–14]. In medical
80 safety, the following changes have been observed over the past 20 years. The idea has
81 rapidly spread worldwide to achieve efficient medical care services with the aid of the
82 popularization of digital imaging and progress in information and communication
83 technology. PACS has become an indispensable image-management system in modern
84 hospitals as it improves convenience and medical efficiency. Several medical images
85 obtained by various modalities are available on a local area network in a hospital or

86 hospital group. Moreover, some images are available on a cloud system, as needed. The
87 volume of medical images has been rapidly increasing, and radiologists and physicians
88 are struggling to keep up with the sheer number of images to review. For most medical
89 images, accurate and reproducible interpretations can be provided by utilizing advanced
90 systems, such as computer-aided diagnosis systems, that can efficiently and correctly
91 gather useful image information based on the quantitative analysis of the image as a
92 diagnostic reference [15].

93 The Institute of Medicine of the National Academy of Sciences in the USA declared its
94 intent to strengthen efforts to prevent medical accidents in the report “To Err is Human:
95 Building a Safer Health System” in November 1999. Since then, various actions have
96 been taken in hospitals for patient safety, not only in the USA, but also worldwide. The
97 most serious mistake in hospitals is the wrong-patient error, which is mainly caused by
98 human errors and can occur in virtually all stages of diagnosis and treatment. The
99 consequences of patient misidentification can be severe, ranging from medical errors to
100 adverse effects on the bottom line. As of 2020, the National Patient Safety Goals effective
101 July 2020 for the hospital program recommends the use of at least two patient identifiers
102 when providing care, treatment, and services to improve the accuracy of patient
103 identification [16]. A key problem with the use of two patient identifiers has been

104 identified [17], and thus, biometrics are to be introduced in clinical care to prevent patient
105 misidentification. However, the ever-increasing number of patient-verification tasks
106 using biometrics to daily workflow increase the burden on healthcare providers, which
107 can result in other human errors or clinical problems in patients. It is believed that the
108 application of biometrics in healthcare can significantly improve both patient
109 convenience and healthcare provider productivity within a short time, thus acting as a
110 solution to the increasing workload. However, it has the following operational concerns
111 for its clinical use. According to the Japan Medical Imaging and Radiological Systems
112 Industries Association (JESRA) guidelines [18], the anonymization of medical images
113 states that “consideration should be given to rare cases with small number of patients and
114 the face as information that can identify the individual.” The image data itself is not
115 considered to be patient-specific information ethically; however, the tag information
116 associated with the medical image is defined as patient-specific information. When
117 biometric information using medical images is introduced, it is supposed that the
118 guidelines and regulations are revised such that the image itself will be subject to patient
119 information protection. It is also necessary to establish a secure environment in practice
120 for the secondary use of patient medical images.

121

122 3. Utilization and evaluation of similar images

123 In the field of computer vision, various methods for retrieving interesting images, such
124 as content-based image retrieval (CBIR) [19], query by image and video content [20], and
125 content-based multimedia information [21], have been utilized to query a specific image
126 on the web or numerous photographs in a database. Although the concept of CBIR, which
127 originated in 1992, is a unique and useful idea to search for similar images, most
128 techniques are based on the examination distance of two images in image-feature spaces,
129 such as the color, shape, and texture of images. Therefore, certain cases did not match in
130 terms of resemblance, as judged by human observers. Muramatsu and Doi investigated
131 similarity measures and methods for the similar image retrieval of breast lesions on
132 mammograms at the beginning of the 21st century. Furthermore, a group at the University
133 of Chicago proposed psychological measures to evaluate similar images [22–27]. Their
134 studies clearly demonstrated the importance of examining the resemblance between
135 medical images.

136

137 4. Image recognition and identification for medical imaging

138 At the end of the 20th century, Morishita *et al.* initiated a study of automated patient
139 recognition and identification for digital chest radiographs (CXRs), and the first paper on

140 this subject was published in 2001 [28]. The study focused on CXRs, which are the most
141 frequent X-ray examinations in hospitals, and was based on a template-matching
142 technique between current and previous CXRs (**Fig. 2 left**) and the histogram analysis of
143 the correlation values that indicate similarity between the CXRs (**Fig. 3**). A thousand pairs
144 of CXRs with an image matrix size of 64×64 for the same patients and different patients
145 were evaluated and exhibited promising results, with a 47.8% correct identification of
146 correct patients without any misidentification as the wrong patients [28]. A comparison
147 of the similarity of the corresponding areas in the two images by evaluating the
148 normalized cross-correlation value and histogram analysis can be used to determine a
149 specific image or similar image in a database that includes several images of the same
150 type [28]. Moreover, it is also possible to reduce the time required to search for a specific
151 patient image from a database containing several images by using a query ranked by
152 image similarities.

153 Transparency to the public about mistakes in image acquisitions was considered taboo
154 until the end of the 20th century; however, after the 1999 academic report by the US
155 Institute of Medicine, such issues have been reported in newspapers and articles in Japan.
156 PACS has evolved over time and has been improved for each hospital environment, which
157 includes access to archive images and links to corresponding patient information. The

158 actual occurrence of filing errors with an initial version of the PACS environment in a
159 hospital was examined in Japan [29]. The implementation of the PACS clearly contributes
160 to a decrease in misfiling errors by healthcare providers. Currently, in Japan, a verification
161 system before images are stored on the PACS server, called the “KENZO system,” is now
162 operating, and misfiling of patients has been reduced considerably. Nevertheless, the
163 wrong-patient problem still occurs occasionally in hospitals because of unavoidable
164 human errors.

165 To further improve the performance of the method developed by Morishita *et al.* [28],
166 edge-enhanced image-based matching [30] (**Fig. 2, middle**) and biological fingerprints
167 (BFs) (**Figs. 2 right and 4**) were applied. The BFs are useful image information that can
168 be used to recognize and identify a specific patient as part of the radiographs [31]. A
169 comparison of the corresponding BFs in two images (current and previous CXRs) is based
170 on the evaluation of the normalized cross-correlation value and histogram analysis.
171 Although the method used a limited number of normal CXRs without abnormalities, it
172 was promising for searching for a specific or similar image in a database containing
173 several similar images. Because BF is a concept that describes the physique, anatomic
174 features, and specific abnormalities of an individual, it can be applied to image matching
175 with other types of radiological imaging.

176 Various BFs on CXRs (**Fig. 4**), namely, whole-lung fields (WLF), cardiac shadows, the
 177 superior mediastinum, lung apices, part of the right lung, and the lower right lung, which
 178 includes the costophrenic angle, were cropped and tested to identify correct and incorrect
 179 patients. The method was based on comparing the BFs in a target CXR to those of other
 180 CXRs in the database [31]. To examine the resemblance for each BF between the current
 181 CXR, $A(i, j)$, and the previous CXR, $B(i, j)$, for the presumed corresponding patient is
 182 determined by the following equation, called the normalized cross-correlation value (C):

$$183 \quad C = \frac{1}{IJ} \sum_{j=1}^J \sum_{i=1}^I \frac{\{A(i,j) - \bar{a}\}\{B(i,j) - \bar{b}\}}{\sigma_A \cdot \sigma_B},$$

184 where

$$185 \quad \bar{a} = \frac{1}{IJ} \sum_{j=1}^J \sum_{i=1}^I A(i, j), \quad \bar{b} = \frac{1}{IJ} \sum_{j=1}^J \sum_{i=1}^I B(i, j),$$

$$186 \quad \sigma_A = \sqrt{\frac{\sum_{j=1}^J \sum_{i=1}^I \{A(i, j) - \bar{a}\}^2}{IJ}}, \quad \sigma_B = \sqrt{\frac{\sum_{j=1}^J \sum_{i=1}^I \{B(i, j) - \bar{b}\}^2}{IJ}}.$$

187 I and J indicate the matrix size of the area selected for each BF of the current images
 188 A and B , respectively. If images A and B are identical, then C is set to 1.0. The correlation
 189 value indicates the resemblance between the two images, where a higher correlation value
 190 indicates a greater similarity. Among several BFs, only a part of the right lung did not
 191 work well for identifying the correct patient owing to fewer differences in image contrasts
 192 in the BF. Then, the sum of the other five correlation values is used as a correlation index
 193 to rank similar images. Finally, a combination of the index and artificial neural networks

194 achieved 58% correct warning rates for different patients.

195 Toge *et al.* improved the overall performance of the correct recognition of the same
196 patients up to 87.5% without incorrect warnings for the same patients by using a
197 weighting factor for each correlation index for the similarity measure. Additionally, an
198 additional 5.0% of the same patients were included in the top-10 ranking of the correlation
199 index in the database [32]. Shimizu *et al.* modified the shape of WLF to improve its
200 performance and applicability for unknown individuals [33] and developed an automatic
201 extraction method for BFs, including the detection of image orientation in digital CXRs
202 [34]. These techniques are introduced in a book entitled *New Perspectives in Forensic*
203 *Human Skeletal Identification* [35] as examples of computer-assisted biometric matching
204 of radiological imaging in non-forensic fields. Kao *et al.* also demonstrated automated
205 patient recognition of CXRs in 2013 [35] by evaluating six characteristics, including the
206 anatomical length and area. The upper part of **Table 1** presents the performance of the
207 automated patient recognition and identification methods using CXRs.

208

209 **5. Patient verification using routine torso CT and brain MR imaging**

210 Cross-sectional imaging systems, such as computed tomography (CT) and magnetic
211 resonance (MR) imaging, are expanding rapidly to become the first-choice examinations

212 for X-ray imaging in several cases. CT and MR imaging produce hundreds to thousands
213 of images per examination. In addition, several CT/MR series images might be sent to an
214 external system for secondary use, or the original dataset may be used for multi-planar
215 reconstruction and volume rendering. Hence, a single wrong-patient registration of an
216 exam could potentially lead to a fatal medical accident. Biometrics in healthcare are
217 preferred as a simple verification/identification task under various patient conditions
218 because routine work for healthcare providers is already complicated.

219 Ueda *et al.* [37, 38] suggested the use of scout images, which are acquired for scan
220 planning purposes, for biometric verification. This makes the examination process
221 convenient for both healthcare providers and patients. The benefits of scout images for
222 biometrics are: high versatility, no additional scanning, and possible automatic execution
223 during an examination. Their use is a novel technique for positive patient verification
224 using routine torso CT and brain MR images. A study entitled “Biological fingerprint
225 using scout computed tomographic images for positive” [37] evaluated the temporal scout
226 CT images of the chest, abdomen, and pelvis scans. In this challenge, the resemblance
227 between the follow-up and baseline images was evaluated by comparing the estimates of
228 the image characteristics using local feature extraction and matching algorithms.

229 **Figure 5** demonstrates the examples of the same- and different-pair analyses using

230 chest–pelvis scout CT images. In this example, the correspondence rates, which are
231 defined as similarity indexes, are 80.6% for the genuine pair and 18.0% for the impostor
232 pair. The highest area under the curve (AUC), equal error rate (EER), and rank-one
233 identification rate (R1) achieved in this study were 0.998, 1.22%, and 99.7%, respectively.

234 Moreover, another study entitled “Usefulness of biological fingerprint in magnetic
235 resonance imaging for patient verification” evaluated eight anatomical multi-planar
236 reconstruction images of the right and left halves of the brain—including the temporal
237 lobe and optic nerve for the sagittal section; optic nerve, optic chiasm, and internal
238 auditory canal (IAC) for the coronal section; IAC, basal ganglia, and lateral fissure for
239 the axial section—and midsagittal images generated from temporal three-dimensional
240 (3D) MR imaging of the brain, as illustrated in **Fig. 6** [38]. In this study, the IAC image
241 exhibited the best performance and yielded AUC, EER, and R1 values of 0.998, 1.37%,
242 and 98.6%, respectively. In this study, the evaluation of the images of patients who
243 underwent surgery between two temporal scans exhibited lower performance; however,
244 those of patients who had undergone surgery before the prior scan exhibited high
245 performance levels, as did those of patients who did not undergo surgery. These methods
246 have the potential to discover the misfiled patient information under/after examination
247 and confirm the patient identity, despite the patient being unable to communicate.

248 The lower part of **Table 1** summarizes the biometric technology using CT and MR
249 imaging. The verification performance for biometrics is evaluated in terms of the receiver
250 operating characteristic (ROC) curve and its corresponding EERs and AUCs. The EER
251 indicates a point that has an equal probability for the misclassification of genuine or
252 impostor pairs on the ROC curve. The lower the value of EER, the better the biometric
253 system is for verification. The close-set identification performance for biometrics was
254 evaluated using R1, which indicates that the rank of the genuine patient pair is higher than
255 that of all the impostor patient pairs. The higher the value of R1, the better the biometric
256 system is for closed-set identification. In a good biometric system, EER, AUC, and R1
257 are low, high, and high, respectively.

258

259 **6. Applications of image recognition and identification in forensic pathology**

260 The personal identification of decedents or human remains has been of important
261 scientific interest for forensic anthropologists to answer legal questions since 1850 [35].
262 The Scientific Working Group for Forensic Anthropology (SWGANTH) [39] and the
263 Organization of Scientific Area Committees for Forensic Science (OSAC)[40] have been
264 working together to systematize, provide best practices for, and develop a consensus
265 standard since 2008. Image matching between postmortem (PM) and antemortem (AM)

266 images is called positive identification and is also used for identification in forensic
267 pathology, where PM and AM images, such as radiography or photography, are compared.
268 Forensic skeletal identification has been researched for a century since Schuller suggested
269 its usefulness in observing the frontal sinus in 1921 [41, 42]. Forensic identification of
270 unknown bodies and human remains using advanced imaging techniques, such as
271 postmortem computed tomography (PMCT), is expected [43–47].

272 Matsunobu *et al.* demonstrated the potential usefulness of the reconstructed two-
273 dimensional (2D) images of ribs and vertebrae from 3D CT images for positive
274 identification of CXRs (**Figs. 7 and 8 c, d**) [48]. Tsubaki *et al.* showed the potential
275 usefulness of sex determination based on morphological features obtained from the 2D
276 CXRs of the ribs and thoracic vertebrae (**Fig. 8 a, b**) [49]. To further utilize CT images
277 for forensic cases, Kawazoe *et al.* proposed an accurate and reproducible semi-automated
278 method to correct the positioning of the brain PMCT compared to that of AMCT, as
279 PMCT positioning is made difficult by covering the corpse with a cadaver bag or changes
280 in rigidity after death (**Fig. 8 e–h**) [50]. For accurate image comparison of the human
281 body, if such correction is installed in the CT system for automatic preprocessing,
282 positioning correction can be easier and more reproducible for operators with different
283 skills.

284 In Japan, the Act of Promotion of Policy about Death Investigation was legislated and
285 enforced in April 2020 to utilize scientific methods to investigate the cause of death and
286 prepare a database for personal identification of corpses [51]. O'Donnell *et al.* identified
287 the potential usefulness of PMCT and MR imaging for personal identification [52].
288 Furthermore, another study reported that whole-body CT images of victims were a valid
289 approach for rapid personal identification during a large fire in Australia in 2009 [53].
290 Interpol established guidelines for disaster-victim identification (DVI) and noted that it
291 was difficult to identify such victims by visual recognition. Therefore, fingerprinting,
292 dental records, DNA profiling, and physical indications are required for conclusive
293 identification [54]. Implanted metals are also important for identifying unknown bodies
294 that are difficult to recognize from visual observations. Wada *et al.* reported a
295 preprocessing method using a CT scout image to check for the existence of implanted
296 metals (**Fig. 8 i**) [55]. Scout images under CT imaging have the advantage of fewer
297 artifacts around the metal implant; therefore, it may be useful for quickly finding metals
298 implanted in the body. Although CT imaging techniques, such as a mobile CT scanner,
299 are required on site, the scout image would be useful in the case of a mass disaster because
300 panoramic dental imaging systems and cone-beam CT, frequently used in dental clinics
301 for dental examination, are unavailable in the field.

302

303 **7. Future expectations and issues**

304 Because most studies on personal identification have used a closed set of cases, with
305 either few cases or only a single case, there is no guarantee of their effectiveness for
306 unknown cases or samples with different conditions. To overcome this problem, as well
307 as to develop a method for personal identification, various types of large databases are
308 required that can be used in the case of mass disasters worldwide.

309 Currently, conventional radiography using screen-film systems in medically advanced
310 countries has almost completely shifted to computed radiography (CR) and flat-panel
311 detectors (FPDs). The number of imaging modalities for medical imaging has increased,
312 and all images are stored digitally. Therefore, various accurate and reproducible image
313 recognition and personal identification are expected to be achieved using automated
314 computer-assisted technologies, including artificial intelligence (AI), as well as image
315 comparison using digital radiography. These changes indicate the requirement for various
316 large databases that can be used for training AIs or positive identification in mass disasters
317 worldwide, as well as in cases of other unidentified persons.

318 The authors concluded that biometrics using advanced medical imaging are the key
319 solutions to the incorrect identification of patients in radiology and the identification of

Review


320 unknown bodies or human remains in forensic pathology.



321


322 **Figure 1.** Schematic illustration of various biometric traits for personal identification

323 and authentication.

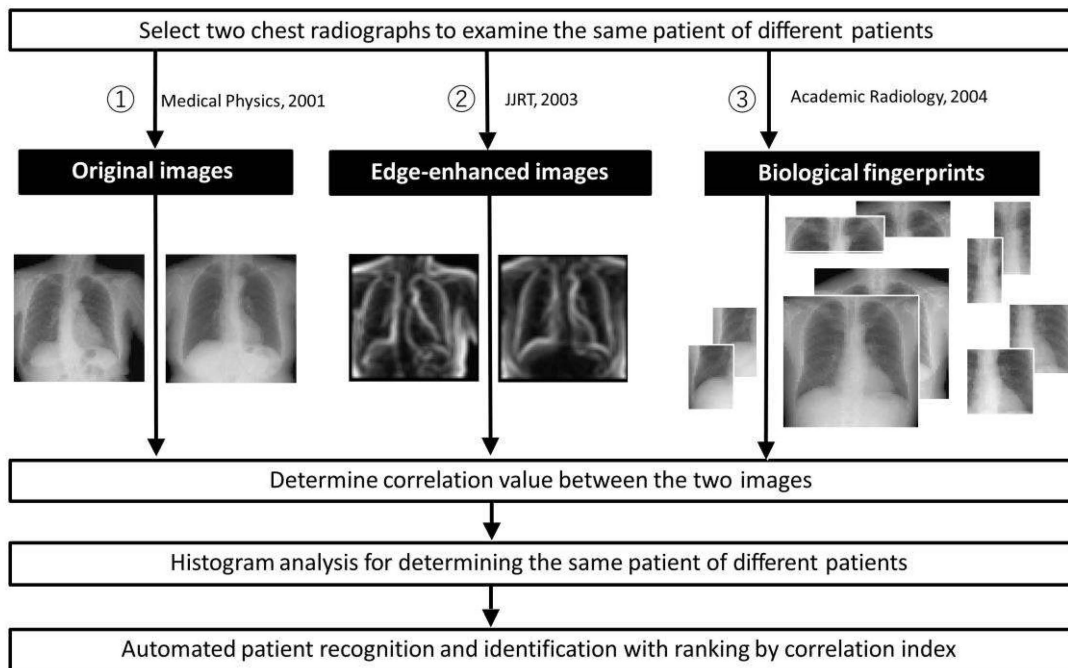

324


325 **Figure 2.** Overall scheme for three different automated patient recognition and
326 identification methods for comparing chest radiographs, based on various template-
327 matching techniques and the histogram analysis of correlation values.

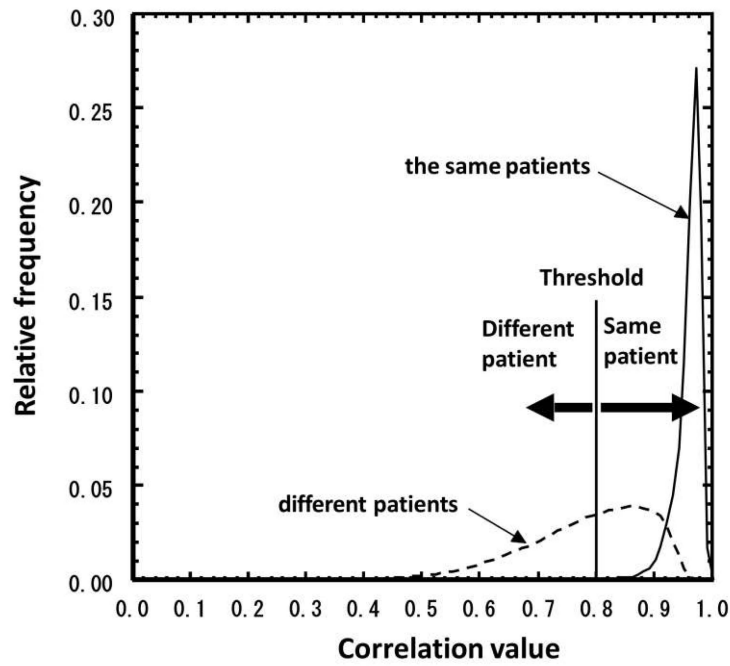

328


329 **Figure 3.** Histograms for correlation values obtained with two chest radiographs for the
330 same patients and for different patients. The threshold value was set at the lowest
331 correlation value for the same patient. However, it can be changed to control the valance
332 of true positives and false negatives.

Review

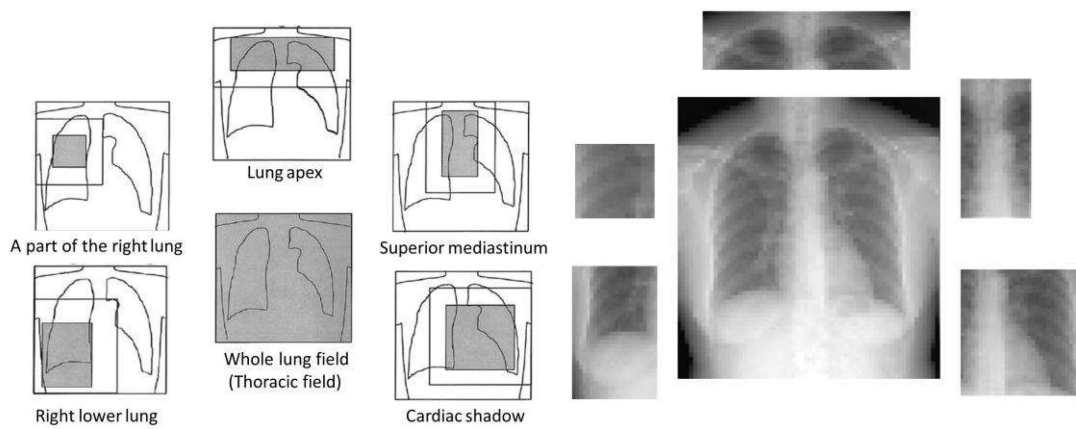

333

334 **Figure 4.** Illustrations of locations for six different BFs, namely, whole-lung field,
335 cardiac shadow, lung apex, the superior mediastinum, part of the right lung, and the
336 lower right lung. The surrounding regions for each BF indicate search areas used in the
337 template-matching technique. An example of BFs extracted from a CXR is shown on
338 the right.




339

340 **Figure 5.** Example of a novel BF technique for biometric verification in CT scout
341 images of the chest, abdomen, and pelvis under a clinical setting. Scout views of follow-
342 up (center) and baseline (right) scans of the same patient are shown. A follow-up
343 (center) and baseline (left) scans corresponding to different patients are shown. Yellow
344 circles indicate the local feature points. Lines connecting pairs of yellow circles in the
345 pairs of images are valid corresponding feature points of the same-patient pair (cyan
346 lines) and different-patients pair (magenta lines). The number of such lines indicates the
347 similarity score. The more the number of lines connecting the feature points, the more

Review

348 likely they are to be the same patient.

349 Note: Original figure adapted from data from Ueda et al. [37].

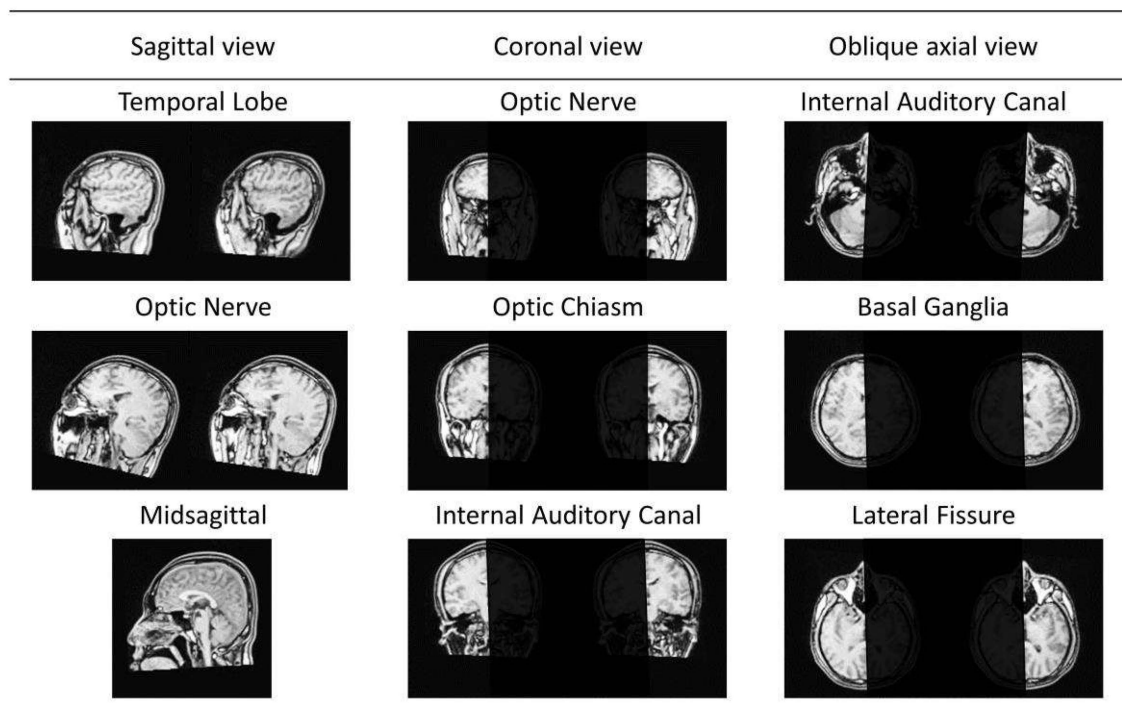

350


351 **Figure 6.** Examples of nine BF images reconstructed from a 3D MR image of the brain.

352 Each 2D BF image was determined comparing each right or left 2D image. The

353 resemblance between the 2D BF images of each identical section was used for biometric

354 verification.

355 Note: Images were adapted from data from Ueda [38].

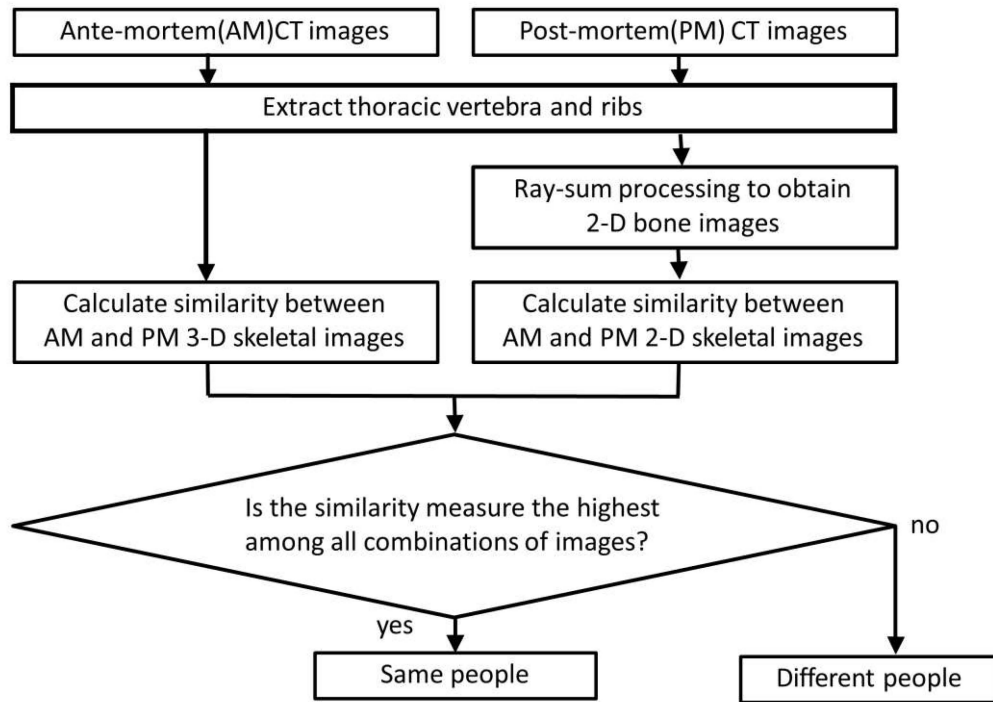


356

357 **Figure 7.** Overall scheme for positive forensic identification using 2D and 3D skeletal

358 images extracted from antemortem (AM) and postmortem (PM) CT images. The

359 normalized cross-correlation value was used as a similarity measure.

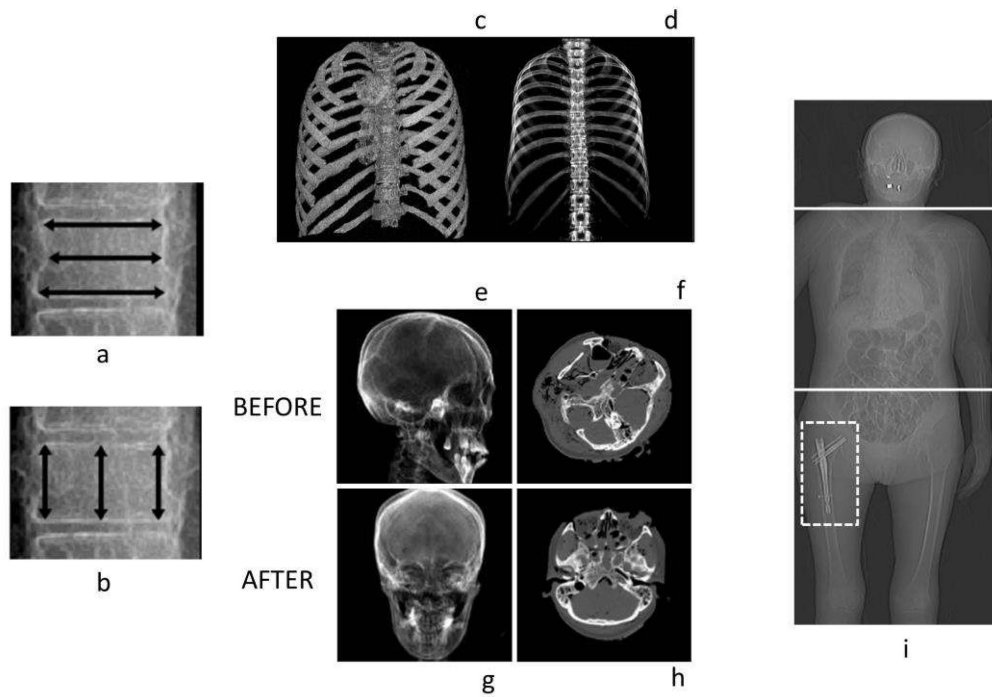

360

361 **Figure 8.** Examples of forensic skeletal identification for sex determination using
 362 thoracic vertebra (a, b), 3D and 2D skeletal images (c, d), head PMCT images before
 363 and after semiautomated position readjustment (e, f, g, h), and an example of three
 364 automatically roughly classified body parts for PMCT scout view, including an artificial
 365 hip joint, as shown in the dashed rectangle (i).

366 **Acknowledgements**

367 The authors are grateful to many individuals for useful discussions the subjects covered
368 in this review, i.e., Noriaki Ikeda, Kunio Doi, Shigehiko Katsuragawa, Yasuo Sasaki,
369 Tadashi Hongyo, Katsuhiko Ueda, Shohei Kudomi, Keiko Kudo, Yosuke Usumoto,
370 Akiko Tsuji, Miki Okumura, and members in Morishita Laboratory. Part of this work was
371 supported by JSPS KAKENHI Grant Numbers JP14570894, JP18591350, JP15K0896,
372 JP19K08122, and JP 18K15590.

Review

373 **Funding**

374 This research was supported in part by JSPS KAKENHI Grant Numbers JP14570894,

375 JP18591350, JP15K0896, JP19K08122, and JP18K15590.

376

377 **Ethics declarations**

378 Conflict of interest

379 All authors declare that they have no conflict of interest.

380

381 Ethical statement

382 All procedures conducted the studies, which involved human participants of introducing
383 in this paper, were in conformance with the ethical standards of the Institutional Review
384 Board at each authors' affiliated institutions and with the 1964 Helsinki Declaration and
385 its later amendments or comparable ethical standards.

386

387 Informed consent

388 Written informed consent of the studies, which involved human participants of
389 introducing in this paper, were not required owing to the retrospective design.

390

391 Animal rights

392 The studies, which are introduced in this paper, did not involve animal model.

393 **References**

- 394 1. Lei G, Liu F, Liu P, Zhou Y, Jiao T, Dang YH. Worldwide tendency and
395 focused research in forensic anthropology: A bibliometric analysis of decade
396 (2008-2017). *Leg Med (Tokyo)*. 2019;37:67-75.
- 397 2. Grew N. The description and use of the pores in the skin of the hands and feet,
398 by the learned and ingenious Nehemiah Grew, M. D. Fellow of the College of
399 physicians and of the Royal Society. *Philosophical Transactions of the Royal*
400 *Society of London*. 1684;14:566-7.
- 401 3. Bidloo G. *Anatomia Humani Corporis*. Amsterdam, Netherlands; 1685.
- 402 4. Mayer JCA. *Anatomical Copper-plates with Appropriate Explanations*; 1788.
- 403 5. Newman HH. Finger prints, palms and soles: An introduction to
404 dermatoglyphics. *American Journal of Physical Anthropology*. 1944;2:227-9.
- 405 6. Herschel W. *The Origin of Finger-Printing*. Oxford: Oxford University Press;
406 1916.
- 407 7. Galton F. *Signaletic Instructions, including the Theory and Practice of*
408 *Anthropometrical Identification*. *Nature*. 1896;54:569-70.
- 409 8. Galton F. *Finger Prints*. London: McMillan; 1892.

- 410 9. Henry ER. Classification and Uses of Finger Prints. London: Routledge; 1900.
- 411 10. Simon A. Cole. Suspect Identities: A History of Fingerprinting and Criminal
412 Identification. London: Harvard University Press; 2001.
- 413 11. United States. The Identification Division of the FBI: A Brief Outline of the
414 History, the Services, and the Operating Techniques of the World's Greatest
415 Repository of Fingerprints. Washington, D.C.: Federal Bureau of Investigation,
416 U.S. Dept. of Justice; 1977.
- 417 12. Dwyer SJ III, Templeton AW, Martin NL, Lee KR, Levine E, Batnitzky S,
418 Rosental S, Preston DF, Price HI, Faszold S, Anderson WH, Cook LT: The cost
419 of managing digital diagnostic images. Radiol, 1982;144:313-8.
- 420 13. Templeton AW, Dwyer SJ III, Templeton AW, Johnson JA, Anderson WH,
421 Hensley KS, Rosenthal SJ, Lee KR, Preston DF, Batnitzky S, Price HI: An on-
422 line digital image management system. Radiol. 1984;152:321-5.
- 423 14. Cox G, Dwyer SJ III, Templeton AW: Computer networks for management in
424 radiology: an overview. CRT Crit Rev Disg Imaging. 1986;25:333-72.
- 425 15. Doi K. Current status and future potential of computer-aided diagnosis in
426 medical imaging. The British J of Radio. 2005:S3-S19.

- 427 16. The Joint Commission. National Patient Safety Goals Effective July 2020 for the
428 Hospital Program, 2020.
429 [https://www.jointcommission.org//media/tjc/documents/standards/national-
430 patient-safetygoals/2020/npsg_chapter_hap_jul2020.pdf](https://www.jointcommission.org//media/tjc/documents/standards/national-
430 patient-safetygoals/2020/npsg_chapter_hap_jul2020.pdf). Accessed 15 Dec 2020.
- 431 17. Henneman PL, Fisher DL, Henneman EA, Pham TA, Campbell MM,
432 Nathanson BH. Patient identification errors are common in a simulated setting.
433 *Ann Emerg Med.* 2010;55:503-9.
- 434 18. Japanese Engineering Standards of Radiological Apparatus. Practical Guide on
435 Handling for Utilization of Medical Image (JESRA TR-0047-2019), 2019,
436 http://www.jira-net.or.jp/publishing/files/jesra/JESRA_TR-0047_2019.pdf.
437 Accessed 15 Dec 2020.
- 438 19. Kato T. Database architecture for content-based image retrieval. *Image Storage
439 and Retrieval Systems.* International Society for Optics and Photonics.
440 1992:112–23.
- 441 20. Flickner M, Sawhney H, Niblack W, Ashley J, Qian Huang, Dom B, Gorkani M,
442 Hafner J, Lee D, Petkovic D, Steele D, Yanker P. Query by image and video
443 content: the QBIC system. *Computer.* 1995;28:23-32.

- 444 21. Lew MS, Sebe N, Djeraba C, Jain R. Content-based multimedia information
445 retrieval: state of the art and challenges. *ACM Trans. Multimedia Comput.*
446 *Commun. Appl.* 2006;2, 1–19.
- 447 22. Muramatsu C, Li Q, Suzuki K, Schmidt RA, Shiraishi J, Newstead GM, Doi K.
448 Investigation of psychophysical measure for evaluation of similar images for
449 mammographic masses: Preliminary results. *Med. Phys.* 2005;32:2295-304.
- 450 23. Muramatsu C, Li Q, Schmidt RA, Suzuki K, Shiraishi J, Newstead GM, Doi K.
451 Experimental determination of subjective similarity for pairs of clustered
452 microcalcifications on mammograms: Observer study results. *Med. Phys.*
453 2006;33:3460-8.
- 454 24. Muramatsu C, Li Q, Schmidt RA, Shiraishi J, Suzuki K, Newstead GM, Doi K.
455 Determination of subjective similarity for pairs of masses and pairs of clustered
456 microcalcifications on mammograms: Comparison of similarity ranking scores
457 and absolute similarity ratings. *Med. Phys.* 2007;34:2890-5.
- 458 25. Muramatsu C, Li Q, Schmidt RA, Shiraishi J, Doi K. Investigation of
459 Psychophysical Similarity Measures for Selection of Similar Images in the
460 Diagnosis of clustered Microcalcifications on Mammograms. *Med. Phys.*
461 2008;35:5695-702.

- 462 26. Muramatsu C, Li Q, Schmidt RA, Shiraishi J, Suzuki K, Newstead GM, Doi K.
463 Determination of similarity measures for pairs of mass lesions on mammograms
464 by use of BI-RADS lesion descriptors and image features, Acad. Radiol.
465 2009;16:443-9.
- 466 27. Li Q, Li F, Shiraishi J, Katuragawa S, Sone S, and Doi K. Investigation of new
467 psychological measures for evaluation of similar images on thoracic CT for
468 distinction between benign and malignant nodules. Med. Phys. 2003;30:2584-
469 93.
- 470 28. Morishita J, Katsuragawa S, Kondo K, Doi K. An automated patient recognition
471 method based on an image-matching technique using previous chest radiographs
472 in the picture archiving and communication system environment. Med Phys.
473 2001;28:1093-7.
- 474 29. Morishita J, Watanabe H, Katsuragawa S, Oda N, Sukenobu Y, Okazaki H,
475 Nakata H, Doi K. Investigation of misfiled cases in the PACS environment and a
476 solution to prevent filing errors for chest radiographs. Acad Radiol. 2005;12:97-
477 103.

- 478 30. Kondo K, Morishita J, Doi K. Katsuragawa. Development of an automated
479 patient recognition method for chest radiographs using edge enhanced images.
480 Jpn J Radiol Technol. 2003;59:1277–84 (in Japanese).
- 481 31. Morishita J, Katsuragawa S, Sasaki Y, Doi K. Potential usefulness of biological
482 fingerprints in chest radiographs for automated patient recognition and
483 identification. Acad Radiol. 2004;11:309-15.
- 484 32. Toge R, Morishita J, Sasaki Y. Doi K. Computerized image searching method
485 for finding correct patients for chest radiographs in a PACS server by use of
486 biological fingerprints. Radiol Phys Technol. 2013;6:437-43.
- 487 33. Shimizu Y, Matsunobu Y, Morishita J. Evaluation of the usefulness of modified
488 biological fingerprints in chest radiographs or patient recognition and
489 identification. Radiol Phys Technol. 2016;9:240-4.
- 490 34. Shimizu Y, Morishita J. Development of a method of automated extraction of
491 biological fingerprints from chest radiographs as preprocessing of patient
492 recognition and identification. Radiol Phys Technol. 2017;10:376-81.
- 493 35. Latham K, Bartelink E, Finnegan M. New Perspectives in Forensic Human
494 Skeletal Identification. Academic Press, 2018.

- 495 36. Kao EF, Lin WC, Jaw TS, Liu GC, Wu JS, Lee CN. Automated patient identity
496 recognition by analysis of chest radiograph features. Acad Radiol.
497 2013;20(8):1024-1031.
- 498 37. Ueda Y, Morishita J, Hongyo T. Biological fingerprint using scout computed
499 tomographic images for positive patient identification. Med Phys.
500 2019;46:4600-9.
- 501 38. Ueda Y, Morishita J, Kudomi S, Ueda K. Usefulness of biological fingerprint in
502 magnetic resonance imaging for patient verification. Med Biol Eng Comput.
503 2016;54:1341-51.
- 504 39. The Scientific Working Group for Forensic Anthropology (SWGANTH): An
505 official web site of the United States government.
506 <https://www.nist.gov/oles/scientific-working-groups/>. Accessed 21 Dec 2020
- 507 40. The Organization of Scientific area Committees for forensic science.
508 [https://www.nist.gov/topics/organization-scientific-area-committees-forensic-](https://www.nist.gov/topics/organization-scientific-area-committees-forensic-science/governing-documents/)
509 [science/governing-documents/](https://www.nist.gov/topics/organization-scientific-area-committees-forensic-science/governing-documents/). Accessed 21 Dec 2020

- 510 41. Shuller A. Das Rontgenogram der Stimhole: ein Hilfsmittel für die
511 Identitätsbestimmung von Schaden. Monatsschrift für Ohrenheilkunde und
512 Laryngo Rhinologie. 1921;5:1617-20 (in German).
- 513 42. Shuller A. A note on the identification of skulls by x-ray pictures of the frontal
514 sinuses. Med J Aust. 1943;1:554-6.
- 515 43. Gowri V R, Adaitya B U. Forensic considerations when dealing with
516 incinerated human dental remains. J Forensic and Legal Med. 2015;29:13-7.
- 517 44. Ciaffi R, Gibelli D, Cattaneo C. Forensic radiology and personal identification
518 of unidentified bodies: a review. Radiol Med. 2011;116:960-8.
- 519 45. Dedouit F, Savall F, Mokrane F-Z, Rousseau H, Crubézy E, Rougé D, Telmon
520 N. Virtual anthropology and forensic identification using multidetector CT. Br J
521 Radiol. 2014;87:20130468.
- 522 46. Kewal K, Preetika M C, Tanuj K, Sandeep K, Neha B. A review of sex
523 estimation techniques during examination of skeletal remains in forensic
524 anthropology casework. Forensic Sci Int. 2016;165:e1-165.
- 525 47. Panchbhai AS. Dental radiographic indicators, a key to age estimation.
526 Dentomaxillofac Radiol. 2011;40:199-212.

- 527 48. Matsunobu Y, Morishita J, Usumoto Y, Okumura M, Ikeda N. Bone
528 comparison identification method based on chest computed tomography
529 imaging. *Legal Medicine*. 2017;29:1-5.
- 530 49. Tsubaki S, Morishita J, Usumoto Y, Sakaguchi K, Matsunobu Y, Kawazoe Y,
531 Okumura M, Ikeda N. Sex determination based on a thoracic vertebra and ribs
532 evaluation using clinical chest radiography. *Legal Medicine*. 2017;27:19-24.
- 533 50. Kawazoe Y, Morishita J, Matsunobu Y, Okumura M, Shin S, Usumoto Y, Ikeda
534 N. A simple method for semi-automatic readjustment for positioning in post-
535 mortem head computed tomography imaging. *Forensic Radiology*. 2019;16:57-
536 64.
- 537 51. Basic act of promotion of death investigation (in Japanese). [https://elaws.e-](https://elaws.e-gov.go.jp/document?lawid=501AC1000000033)
538 [gov.go.jp/document?lawid=501AC1000000033](https://elaws.e-gov.go.jp/document?lawid=501AC1000000033). Accessed 21 Dec 2020.
- 539 52. O'Donnel C, Woodford N. Post-mortem radiology - a new sub-speciality?
540 *Clin Radiol*. 2008;63:1189-94.
- 541 53. O'Donnel C, Iino M, Mansharan K, Mansharan K, Leditscke J, Woodford N.
542 Contribution of postmortem multidetector CT scanning to identification of the

- 543 deceased in a mass disaster: Experience gained from the 2009 Victorian
544 bushfires. *Forensic Science International*. 2011;205:15-28.
- 545 54. INTERPOL. Guideline for disaster victims identification (DVI). In: Interpol.
546 2018. <https://www.interpol.int/How-we-work/Forensics/Disaster-Victim->
547 Identification-DVI. Accessed 22 Dec 2020.
- 548 55. Wada Y, Morishita J, Yoon Y, Okumura M, Ikeda N. A simple method for the
549 automated classification of body parts and detection of implanted metal using
550 postmortem computed tomography scout view. *Radiol Phys Technol*.
551 2020;13:378-84.
- 552